© 2026 Medi-Rent Pty Limited

REJUVI8 QUICK SET-UP GUIDE: LEG

This guide is intended as a quick reference once the user manual has been read in-full

Medi-Rent Pty Limited
ABN: 37 603 454 360
info@medirent.com.au

AU PH: 1300 726 666

HEAD OFFICE:
Unit 1, 61 Beauchamp Rd
Matraville NSW 2036

Unit 2, 2 Carrington Drive,
Albion VIC 3020

Unit 3, 8 Emplacement Crescent
Hamilton Hill WA 6163

Unit 5, 209 Robinson Rd East
Geebung, QLD 4034

NZ PH: 0800 725 555

9F Lady Ruby Drive
East Tamaki
Auckland 2013
NEW ZEALAND

www.medirent.com.au
www.medirent.co.nz

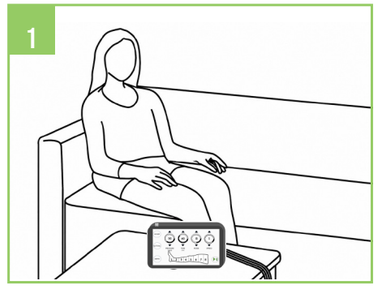

Place the device somewhere easily accessible. It is recommended that you wear light-weight clothing under the Rejuvi8 sleeve.

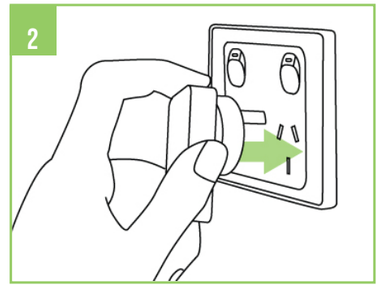

Rejuvi8 can run on battery or plugged into mains power. Ensure leads and hosing do not create a trip hazard. You may need to visit the bathroom during treatment due to fluid drainage.

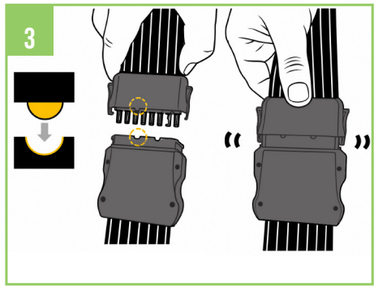

To connect the hosing in the correct direction, align the raised bumps on the hosing connector with notches of the connection.
1 sleeve: Connect hosing directly to the device connnector, press the pieces together.
2 sleeves: Connect sleeve hoses to the adapter* and the adapter to the device. You should hear a “CLICK” sound when connected correctly.

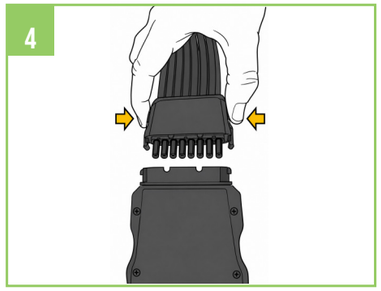

To disconnect hosing- press the tabs on either side of the hosing and pull

Adapter



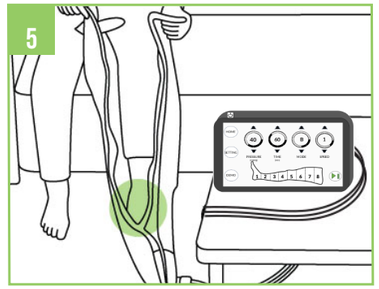

Place your leg into the sleeve by unzipping it part-way.

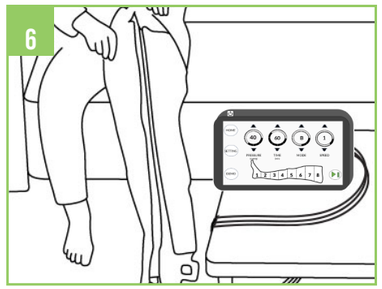

Fasten cuff zip and Velcro tabs.

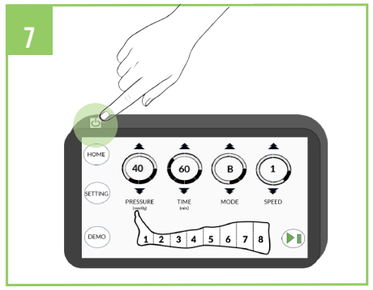

Turn the device on by pressing “Power”.

Superior compression rejuvi8 made simple

MEDI-RENT
THE MEDICAL EQUIPMENT RENTAL SPECIALISTS

8

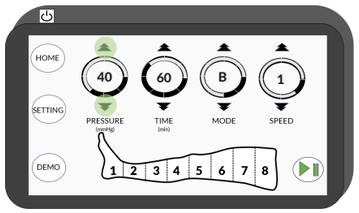

PRESSURE- Firmness of the sleeve when inflated. A higher value will have firmer compression.

TIME- This is the session duration. The device will run for the set time and then stop. Countdown timer is on the top right of the display.

MODE- Inflation sequence of air chambers. Enter the DEMO screen to view the modes.

SPEED- This is the cycle time for the device to inflate and deflate. Speed 1 is the quickest cycle, speed 5 is the slowest cycle

Adjust the settings to match those prescribed by your healthcare professional.

To adjust Pressure/Time/Mode/Speed:
Tap the arrows above or below each setting to change the value.

9

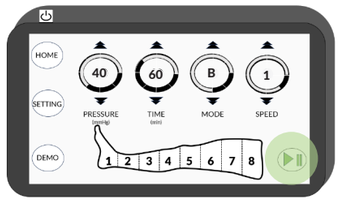

If no settings have been prescribed, start with the settings displayed above. Press the Start button to begin therapy.

Pressure 40mmHg
Time 60min
Mode B
Speed 1

To stop therapy at any time, press the Play/Pause button again.

10

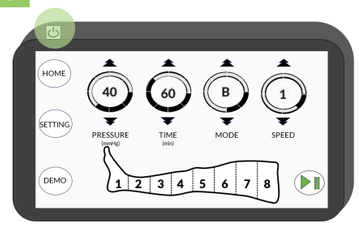

When therapy is complete, turn off the power button and unzip your garment. Plug the Rejuvi8 device into mains power to charge.

** *Select the DEMO screen to view Set-Up videos.*

Or scan the QR code to view our complete set-up video.

11

Whilst the compression pump is running please read the **'Settings Navigation Guide.'**

Allow the device run for at least 10 minutes after each change for the full effect to be felt.

12

If you wish to clean the garment at any time, simply use warm soapy water or Clinell wipes. These specific cleaning wipes do not contain alcohol like many other sanitising wipes which can damage the garments. Do not place in washing machine or dryer.

WARNING

* **Be advised by your Health Professional on setting selection, pressure and duration.**

** Always check your body for any pressure areas after treatment. If using the pump for prolonged periods adhere to pressure area prevention techniques such as changing position regularly and sitting/lying on a supportive surface.

CONTRAINDICATIONS FOR USING A COMPRESSION PUMP

* Known or suspected deep vein thrombosis
* Pulmonary embolism
* Thrombophlebitis
* Cellulitis or other infection not treated with antibiotics
* Uncontrolled/severe cardiac failure
* Pulmonary oedema
* Active metastatic disease affecting oedematous region

IF YOU CHOOSE TO USE THE REJUVI8 WITH ANY OF THE ABOVE CONDITIONS YOU MUST DO SO UNDER THE SUPERVISION OF YOUR TREATING HEALTH PROFESSIONAL.

HAVE QUESTIONS?

Call us on **AU PH 1300 726 666** or **NZ PH 0800 725 555**

© 2026 v1